

All data taken at the Pacific Northwest National Laboratory  
FTS Operators: Tyler O. Danby and Paul L. Gassman  
Data Analysis: Russell G. Tonkyn, Jerome C. Birnbaum, and Molly Rose K. Kelly-Gorham

**Composite spectrum for:** 1,4-Thioxane

- First Column: Position in wavenumber ( $\text{cm}^{-1}$ )
- Second column: Real refractive index  $n(\tilde{\nu})$  (dispersion index)
- Third column: Imaginary refractive index,  $k(\tilde{\nu})$  (absorption index per unit length in centimeters)

Where the complex refractive index  $\hat{n} = n(\tilde{\nu}) + ik(\tilde{\nu})$

Following Bertie (in the references below) we define the absorbance as  $A = -\log_{10}(I/I_0)$  and the linear absorption coefficient  $K = A/d$ , where  $d$  is the path length. The connection between the imaginary refractive index and the absorbance coefficient arises from the following:  $2.303K = 4\pi\tilde{\nu}k$

See the following references for a detailed description of terms and units:

- 1) Bertie, J. E., Zhang, S. L., Eysel, H. H., Baluja, S., & Ahmed, M. K. (1993). Infrared Intensities of Liquids XI: Infrared Refractive Indices from 8000 to  $2\text{ cm}^{-1}$ , Absolute Integrated Intensities, and Dipole Moment Derivatives of Methanol at  $25^\circ\text{C}$ . *Applied Spectroscopy*, 47(8), 1100-1114. doi:10.1366/0003702934067973
- 2) Bertie, J. E., Zhang, S. L., & Keefe, C. D. (1995). Measurement and use of absolute infrared absorption intensities of neat liquids. *Vibrational Spectroscopy*, 8(2), 215-229. doi:10.1016/0924-2031(94)00038-i

**Sample:**

- Chemical name, formula and CAS number: 1,4-Thioxane,  $\text{C}_4\text{H}_8\text{OS}$ , [15980-15-1]
- IUPAC name: 1,4-Thioxane
- Synonyms: 1,4-Oxathiane
- Physical properties: FW = 104.17 g/mole; mp =  $-21.5^\circ\text{C} - -16.9^\circ\text{C}$ ; bp =  $147^\circ\text{C}$ ;  $\rho = 1.114\text{ g/cm}^3$
- Supplier and stated purity: Aldrich, 98% (Lot # MKBL9069V)
- Temperature of sample:  $26^\circ\text{C}$  ( $\pm 1^\circ\text{C}$ )
- Individual samples were measured at the following path lengths: 2.6, 4.4, 15.2, 35.8, 53.2, 102, 202, 505 and 1230 micrometers ( $\mu\text{m}$ ). Final data are a composite of these spectra.
- Sample cell window material is potassium bromide (KBr).
- Preparation: None.
- Sample likely has trace amounts of water.

**Instrument Parameters:**

- Bruker Tensor 27 FTIR, purged with UHP nitrogen
- Spectral range:  $7800$  to  $400\text{ cm}^{-1}$  (1.282 to 25 microns)
- Instrument resolution:  $2.0\text{ cm}^{-1}$
- Number of interferograms averaged per single channel spectrum: 128
- Apodization: Norton-Beer, Medium
- Phase correction: Mertz
- Scanner velocity: 10 kHz
- Folding limits:  $15802$  to  $0\text{ cm}^{-1}$
- Interferogram zerofill: 4x
- Spectral interval after zerofilling:  $0.4823\text{ cm}^{-1}$
- IR source: Silicon carbide glow bar
- Beamsplitter: Broadband potassium bromide (KBr)
- Detector: DLTGS at room temperature
- Aperture: 3 mm

### Measured Refractive Index:

The refractive Index for 1,4-Thioxane was measured at 27 °C using an Atago model DR-M2/1550 Abbe refractometer. Notch filters were employed in front of a white light source to make measurements at multiple wavelengths. An InGaAs camera was used to detect signal at 1550 nm. The temperature was controlled to match that in the sample compartment of the FTIR using a heated circulating bath.

480 nm: $n = 1.5113$	486 nm: $n = 1.5106$	546 nm: $n = 1.5052$
589 nm: $n = 1.5025$	644 nm: $n = 1.4999$	656 nm: $n = 1.4994$
1550 nm: $n = 1.4884$		

The refractive index,  $n$ , vs. wavelength in microns,  $\lambda$ , was fit to an equation similar to that of Sellmeier:

$$n(\lambda) = \{a + b/(\lambda^2 - c)\}^{1/2}$$

The resulting best-fit equation was used to find the refractive index at the highest energy data point in our experimental spectra. For 1,4-Thioxane, the result was

$$n(7800 \text{ cm}^{-1}) = 1.4895 \text{ at } 27 \text{ }^\circ\text{C}.$$

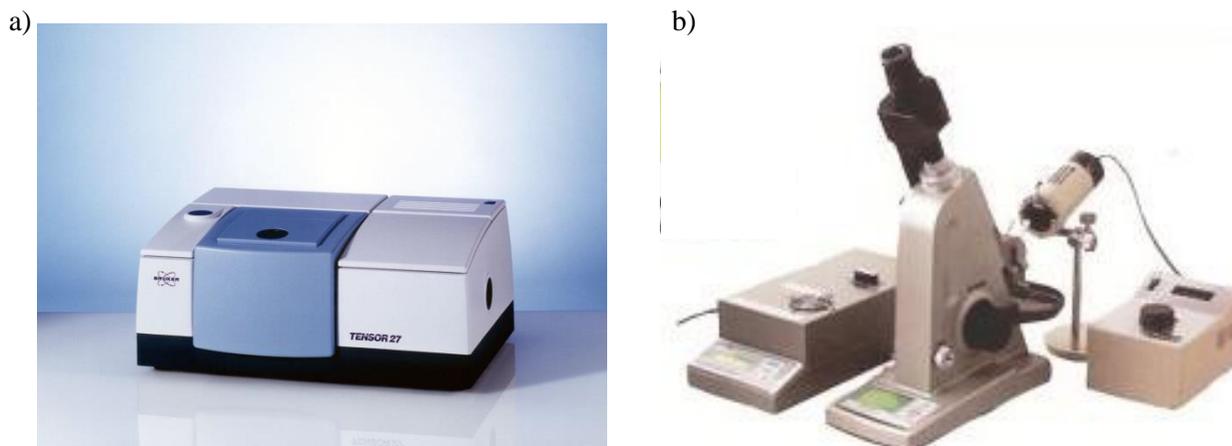


Figure 1: The Bruker Tensor 27 FTIR (a) and Abbe refractometer (b).

### Post Processing and Related Parameters:

A composite spectrum was created from 9 absorbance spectra (base-10) taken at 9 path lengths: 2.6, 4.4, 15.2, 35.8, 53.2, 102.2, 202, 505 and 1230 micrometers ( $\mu\text{m}$ ). At each path length several spectra were measured and the results averaged for better signal to noise. The measured cell lengths were adjusted using Beer's law plots.

- 1) The imaginary part of the refractive index, or  $k$  vector, was determined for each absorbance file as per Bertie's program "RNJ46A" (see reference above). This takes into account the reflective losses due to the KBr windows.
- 2) A composite  $k$  vector is created via a classical, weighted, linear, least squares fit using the output files of program "RNJ46A": Intercept=0, slope is fitted, individual absorbance values weighted by  $T^2$  (transmission squared), all absorbance values  $\geq 2.5$  are given zero weight. Six composite vectors were created and merged by hand.
  - a) The first  $k$  vector used the results from the 1230 and 505  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 7800 to 4500  $\text{cm}^{-1}$ , 3900 to 3540  $\text{cm}^{-1}$  and 1800 to 1475  $\text{cm}^{-1}$ .
  - b) The second  $k$  vector used the results from the 505 through 102  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 4500 to 3900  $\text{cm}^{-1}$ , 3540 to 3000  $\text{cm}^{-1}$  and 540 to 400  $\text{cm}^{-1}$ .
  - c) The third  $k$  vector used the results from the 15 through 3  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 3000 to 2795  $\text{cm}^{-1}$ , 830 to 818  $\text{cm}^{-1}$  and 540 to 400  $\text{cm}^{-1}$ .

- d) The fourth  $k$  vector used the results from the 15 through 3  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 2795 to 1800  $\text{cm}^{-1}$ .
  - e) The fifth  $k$  vector used the results from the 53 through 3  $\mu\text{m}$  cells. This  $k$  vector determined the final values for the range from 1475 to 1290  $\text{cm}^{-1}$ , 1275 to 1110  $\text{cm}^{-1}$ , 1090 to 1010  $\text{cm}^{-1}$ , 990 to 830  $\text{cm}^{-1}$  and 818 to 560  $\text{cm}^{-1}$ .
  - f) The sixth  $k$  vector used the results from the 4 and 3  $\mu\text{m}$  cells. This  $K$  vector determined the final values for the range from 1290 to 1275  $\text{cm}^{-1}$ , 1110 to 1090  $\text{cm}^{-1}$  and 1010 to 990  $\text{cm}^{-1}$ .
- 3) The resulting composite  $k$  vector and the refractive index at 7800  $\text{cm}^{-1}$  were used to create the real or  $n$  vector using the Kramers-Kronig relation, as per Bertie's program "LZZKTB."
- a) Calculated and estimated errors: Type A = 0.7%.
  - b) Frequency correction (already applied):  $\tilde{\nu}(\text{corrected}) = [\tilde{\nu}(\text{instrument}) * .99975 + .003891]$  as determined by comparing measured atmospheric spectral lines ( $\text{H}_2\text{O}$  and  $\text{CO}_2$ ) to values from the Northwest Infrared Spectral Library Database.
  - c) Axis units: X = Wavenumbers ( $\text{cm}^{-1}$ ); Y = Absorbance (base 10).

### Photograph of Sample 1,4-Thioxane:

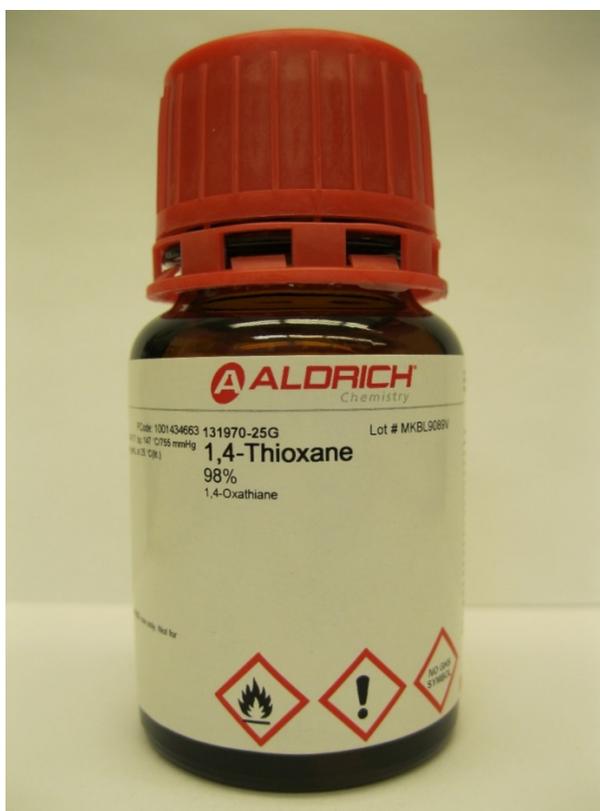


Figure 2: 1,4 Thioxane in Aldrich container.