All data taken at the Pacific Northwest National Laboratory

FTS Operators: Tyler O. Danby and John S. Loring

Data Analysis: Russell G. Tonkyn and Jerome C. Birnbaum

Composite spectrum for: Glyoxal solution

• First Column: Position in wavenumber (cm⁻¹)

• Second column: Real refractive index $n(\tilde{v})$ (dispersion index)

• Third column: Imaginary refractive index, $k(\tilde{v})$ (absorption index per unit length in centimeters)

Where the complex refractive index $\hat{n} = n(\tilde{v}) + ik(\tilde{v})$

Following Bertie (in the references below) we define the absorbance as $A = -\log_{10}(I/I_0)$ and the linear absorption coefficient K = A/d, where d is the path length. The connection between the imaginary refractive index and the absorbance coefficient arises from the following: $2.303K = 4 \pi \tilde{v} k$

See the following references for a detailed description of terms and units:

- 1) Bertie, J. E., Zhang, S. L., Eysel, H. H., Baluja, S., & Ahmed, M. K. (1993). Infrared Intensities of Liquids XI: Infrared Refractive Indices from 8000 to 2 cm⁻¹, Absolute Integrated Intensities, and Dipole Moment Derivatives of Methanol at 25°C. *Applied Spectroscopy*, 47(8), 1100-1114. doi:10.1366/0003702934067973
- 2) Bertie, J. E., Zhang, S. L., & Keefe, C. D. (1995). Measurement and use of absolute infrared absorption intensities of neat liquids. *Vibrational Spectroscopy*, 8(2), 215-229. doi:10.1016/0924-2031(94)00038-i

Sample:

- Chemical name, formula and CAS number: Glyoxal solution, C₂H₂O₂, [107-22-2]
- IUPAC name: Ethanedial
- Synonyms: Ethanedione; Oxalaldehyde
- Physical properties: FW = 58.04 g/mole; mp = 15 °C; bp = 51 °C; ρ = 1.27 g/cm³.
- Supplier and stated purity: Sigma-Aldrich, 40 wt.% in H₂O (Lot # MKBV9169V)
- Temperature of sample: 26 °C (+/-1 °C)
- Individual samples were measured at the following path lengths: 2.8, 3.0, 5.7, 27, 52, 104, 200, 514 and 1008 micrometers (µm). Final data are a composite of these spectra.
- Sample cell window material is zinc selenide (ZnSe).
- Preparation: None.

Instrument Parameters:

- Bruker Tensor 27 FTIR, purged with UHP nitrogen
- Spectral range: 7800 to 400 cm⁻¹ (1.282 to 25 microns)
- Instrument resolution: 2.0 cm⁻¹
- Number of interferograms averaged per single channel spectrum: 128
- Apodization: Norton-Beer, Medium
- Phase correction: Mertz
- Scanner velocity: 10 kHz
- Folding limits: 15802 to 0 cm⁻¹
- Interferogram zerofill: 4x
- Spectral interval after zerofilling: 0.4823 cm⁻¹
- IR source: Silicon carbide glow bar
- Beamsplitter: Broadband potassium bromide (KBr)
- Detector: DLTGS at room temperature
- Aperture: 3 mm

Measured Refractive Index:

The refractive index for Glyoxal solution was measured at 27 °C using an Atago model DR-M2/1550 Abbe refractometer. Notch filters were employed in front of a white light source to make measurements at multiple wavelengths. An InGaAs camera was used to detect signal at 1550 nm. The temperature was controlled to match that in the sample compartment of the FTIR using a heated circulating bath.

480 nm: n = 1.412 486 nm: n = 1.4118 546 nm: n = 1.408 589 nm: n = 1.4064 644 nm: n = 1.4049 656 nm: n = 1.4044

1550 nm: n = 1.3883

The refractive index, n, vs. wavelength in microns, λ , was fit to an equation similar to that of Sellmeier:

$$n(\lambda) = \{a + b/(\lambda^2 - c)\}^{1/2}$$

The resulting best-fit equation was used to find the refractive index at the highest energy data point in our experimental spectra. For Glyoxal solution, the result was

$$n(7800 \text{ cm}^{-1}) = 1.3907 \text{ at } 27 \text{ }^{\circ}\text{C}.$$

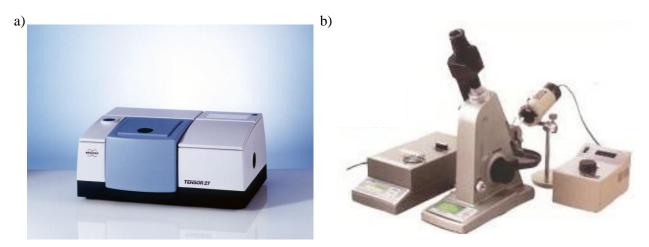


Figure 1: The Bruker Tensor 27 FTIR (a) and Abbe refractometer (b).

Post Processing and Related Parameters:

A composite spectrum was created from 9 absorbance spectra (base-10) taken at 9 path lengths: 2.8, 3.0, 5.7, 27, 52, 104, 200, 514 and 1008 micrometers (µm). At each path length several spectra were measured and the results averaged for better signal to noise. The measured cell lengths were adjusted using Beer's law plots. The large refractive index of ZnSe resulted in considerable fringing in the spectra. In the spectra, the fringe amplitudes and wavelengths varied versus wavenumber, and the baseline slope varied. These effects made it difficult to remove the fringes in a single systematic step. Instead they were removed either by smoothing or by sequentially fitting regions of the baseline to polynomials that passed through the "zero crossings" of the fringes. This process is inherently subjective, particularly on or near absorption peaks. In addition, absorption increases for ZnSe at wavenumbers below 550 cm⁻¹ resulting in increased noise; thus the data is truncated at 500 cm⁻¹.

- 1) The imaginary part of the refractive index, or *k* vector, was determined for each absorbance file as per Bertie's program "RNJ46A" (see reference above). This takes into account the reflective losses due to the ZnSe windows.
- 2) A composite *k* vector is created via a classical, weighted, linear, least squares fit using the output files of program "RNJ46A": Intercept=0, slope is fitted, individual absorbance values weighted by T² (transmission squared), all absorbance values ≥ 2.5 are given zero weight. Four composite vectors were created and merged by hand.

- a) The first k vector used the results from the 104, 200, 514 and 1008 μ m cells. This k vector determined the final values for the range from 7800 to 3700 cm⁻¹.
- b) The second k vector used the results from the 2.8 and 3.0 μ m cells. This k vector determined the final values for the range from 3700 to 3100 cm⁻¹.
- c) The third k vector used the results from the 27, 52 and 104 μ m cells. This k vector determined the final values for the range from 3100 to 1700 cm⁻¹.
- d) The fourth k vector used the results from the 2.8, 3.0, 5.7, 27 and 52 μ m cells. This k vector determined the final values for the range from 1700 to 400 cm⁻¹.
- 3) The resulting composite *k* vector and the refractive index at 7800 cm⁻¹ were used to create the real or *n* vector using the Kramers-Kronig relation, as per Bertie's program "LZZKTB."
 - a) Calculated and estimated errors: Type A = 0.7%.
 - b) Frequency correction (already applied): $\tilde{v}(\text{corrected}) = [\tilde{v}(\text{instrument}) * .99977 0.01872]$ as determined by comparing measured atmospheric spectral lines (H₂O and CO₂) to values from the Northwest Infrared Spectral Library Database.
 - c) Axis units: $X = Wavenumbers (cm^{-1})$; Y = Absorbance (base 10).

Photograph of Sample Glyoxal solution:



Figure 2: Glyoxal solution in Sigma-Aldrich container.