

All data taken at Pacific Northwest National Laboratory (PNNL)

**Operators:** Jerome C. Birnbaum, Tyler O. Danby, Timothy J. Johnson, Molly Rose K. Kelly-Gorham, Rodica Lindenmaier, Tanya L. Myers

**SAMPLE CONDITIONS & PHYSICAL PROPERTIES**

Chemical name	Sodium chlorate	
Chemical formula	NaClO <sub>3</sub>	
Synonyms	n/a	
CAS number	7775-09-9	
Location of field sample	n/a	
History of sample	n/a	
Molecular Weight	106.44 g/mole	
Melting Point	248 - 261 °C	
Boiling Point	n/a	
Density (20 °C)	2.490 g/cm <sup>3</sup>	
Hardness, Mohs scale	n/a	
Crystallography:		
Cell dimension	a = Å b = Å c = Å	
Crystal system		
H-M symbol (point gr)		
Space group		
H-M symbol (space gr)		
Crystal habit		
Color	White	
Diaphaneity	Translucent to sub-translucent	
Particle size	192 ± 159 µm	
Particle size assessment	Optical microscopy	
Supplier	Sigma-Aldrich	
Stated purity	≥ 99.0%	
Date packed	10 October 2016	Weight: 3.137 grams
Synthesis method	n/a	
Synthesis reference	n/a	
Texture	Hygroscopic crystals that clump	
Physical state	Solid	
Surface roughness	n/a	
Elemental composition	n/a	
Isotopic composition	n/a	
Moisture content	n/a	
Temperature of sample	21 ± 2 °C	
Substrate	none	

## INSTRUMENT PARAMETERS

### Tensor 37 FT-IR manufactured by Bruker Optics

External diffuse reflectance accessory	A 562-G integrating sphere
Sphere diameter	75 mm
Angle to normal incidence	14.8°
Sphere opening diameter	19 mm (entrance port)
Spectral range	7,500 to 600 cm <sup>-1</sup> saved; 7500 to 600 cm <sup>-1</sup> reported
Beamsplitter	Ge on KBr
Detector (dia. Det. Port in sphere)	2×2 mm, 60° field of view MCT (550; 0.9); 1 cm
Apodization function	Blackman-Harris 3-term
Aperture	6 mm
Coadded scans	2048
Scanner speed	40 kHz
Switch gain on	512 points
Low pass filter	Open
Scan technique	double-sided, forward-backward
Non-linear correction	Off
High and low folding limit	15802.38-0.00 cm <sup>-1</sup>
Phase resolution	32.00
Phase correction mode	Mertz
Zerofilling	4×
Wavenumber accuracy	± 0.4 cm <sup>-1</sup>
Spectral resolution	4 cm <sup>-1</sup>
Accuracy verification	10/28/2015
Wavelength vetted on:	ICL polystyrene standard #0009-7394-0025A, thin film
Reflectance:	±2% using SRS reflectance standards 50-010-DH27B-4878

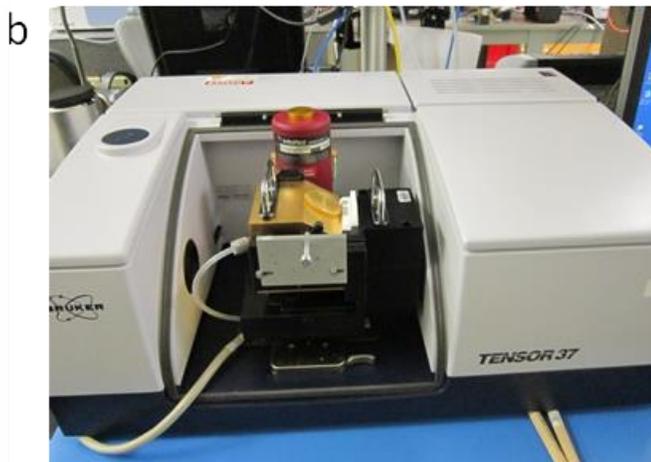
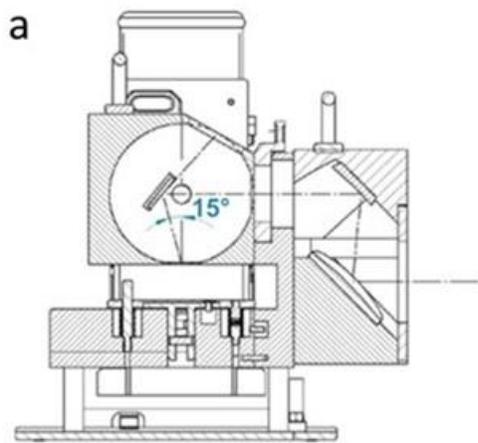


Figure 1: The Bruker 562-G integrating sphere (a) and Tensor 37 (b)

Photographs of sample Sodium chlorate



Figure 2: Sodium chlorate in Sigma-Aldrich container.

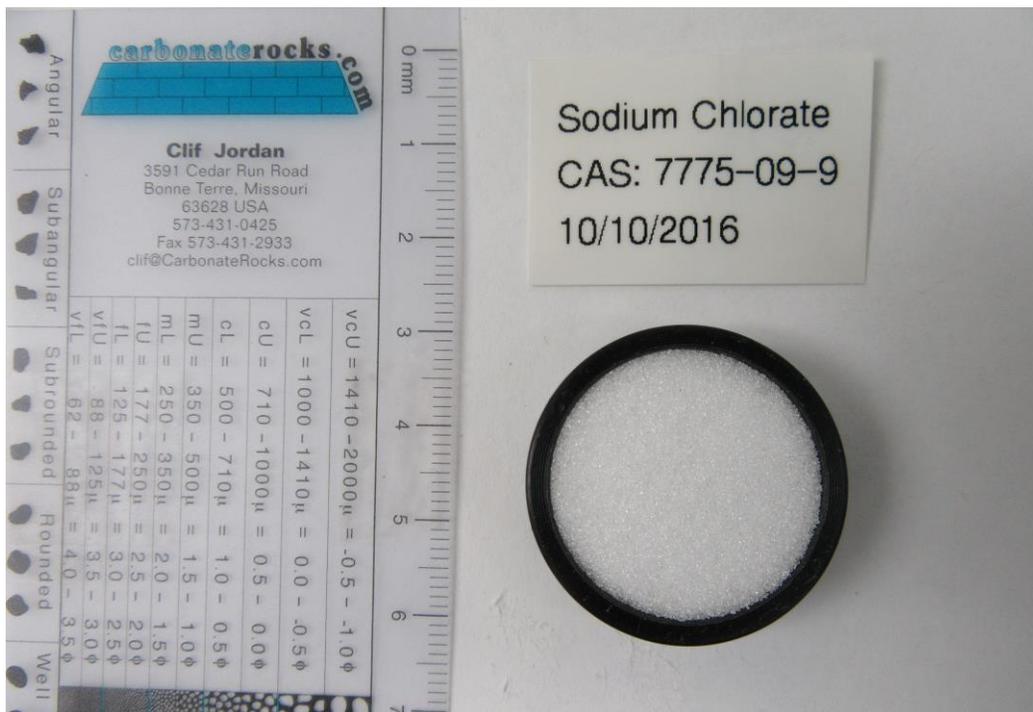


Figure 3: Sodium chlorate loaded in IR sample cup.

## PARTICLE SIZE PREPARATION AND CHARACTERIZATION

### Optical microscopy —

A Keyence VHX-1000 digital microscope with 16-bit resolution is used to provide photomicrographs of the various samples and particle sizes. Software included with the microscope differentiates the brightness and colors in the image and extracts the bright objects to produce a binary image. The software assumes all adjacent bright points are part of the same object then calculates the area for each of these objects. The area (A) is used to calculate the mean particle diameter (d) by assuming the particles are spherical and using the relationship  $d = \sqrt{4A/\pi}$ . Although the assumption of spherical particles is clearly not always valid, this procedure provides a reasonable estimate of the mean particle size.

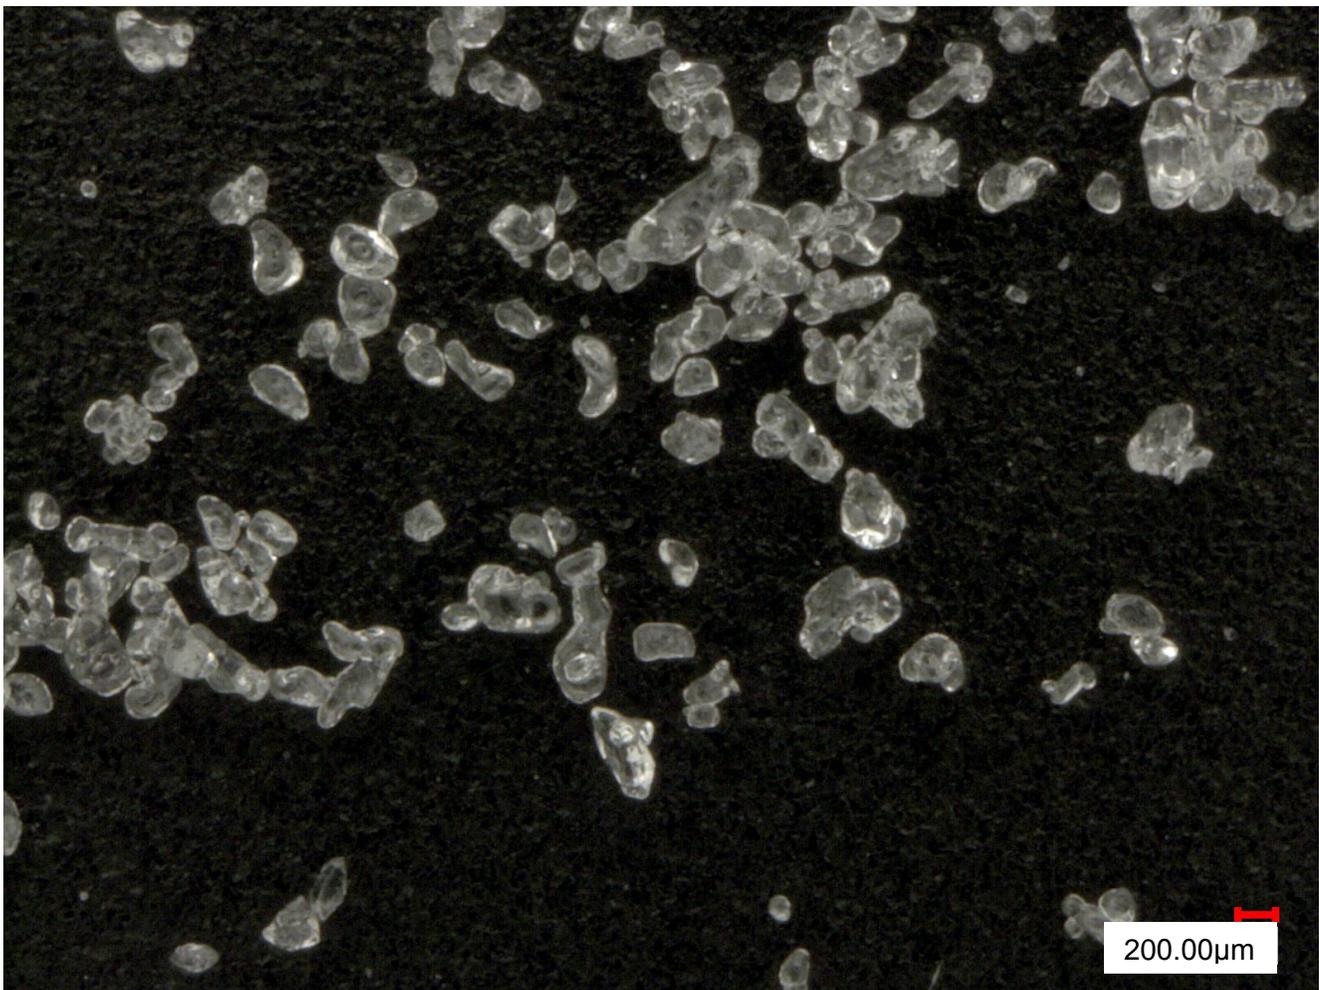


Figure 4: Photomicrograph of Sodium chlorate.

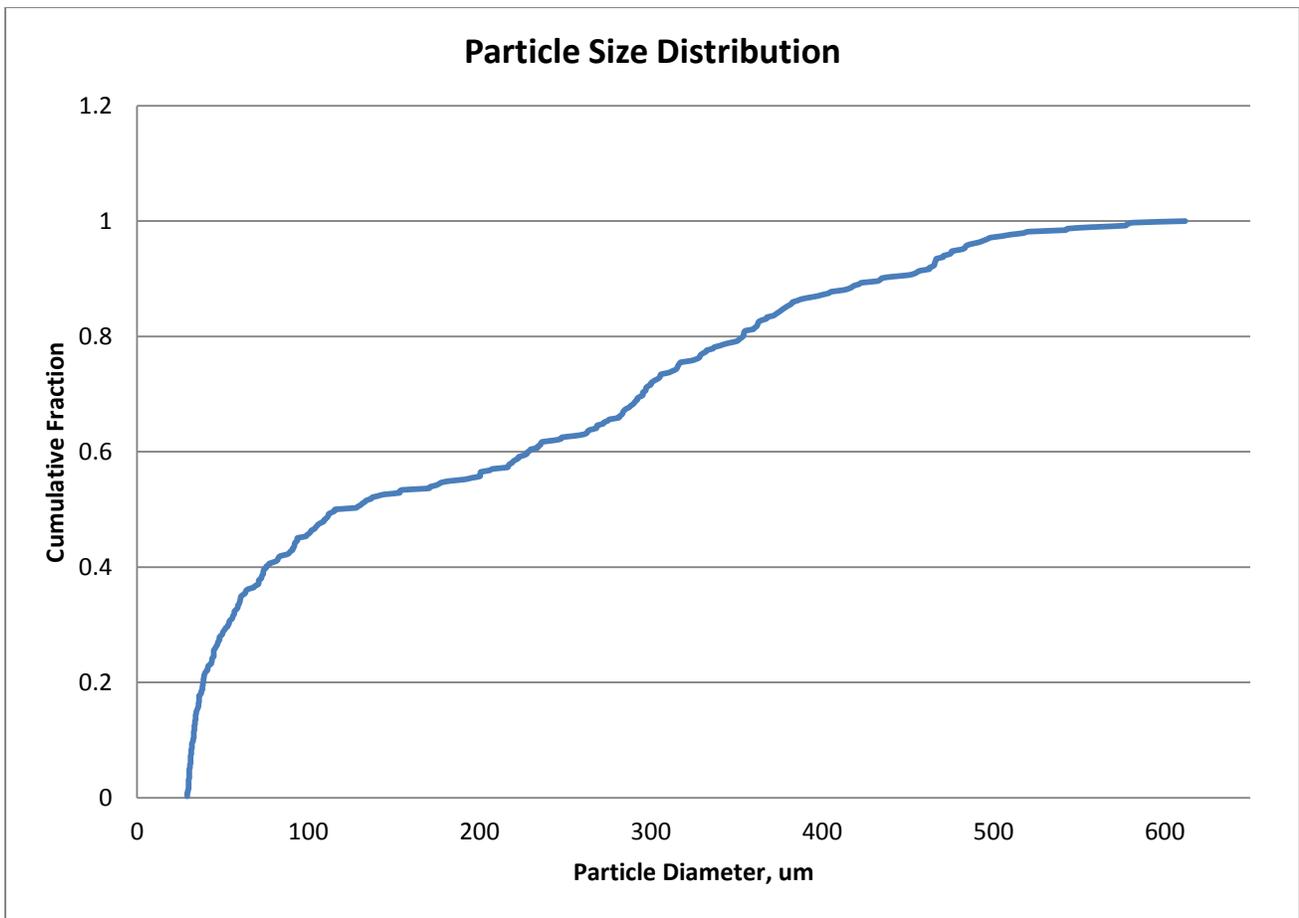


Figure 5: Particle size distribution of Sodium chlorate.